


Plant aneuploidy using flow cytometry

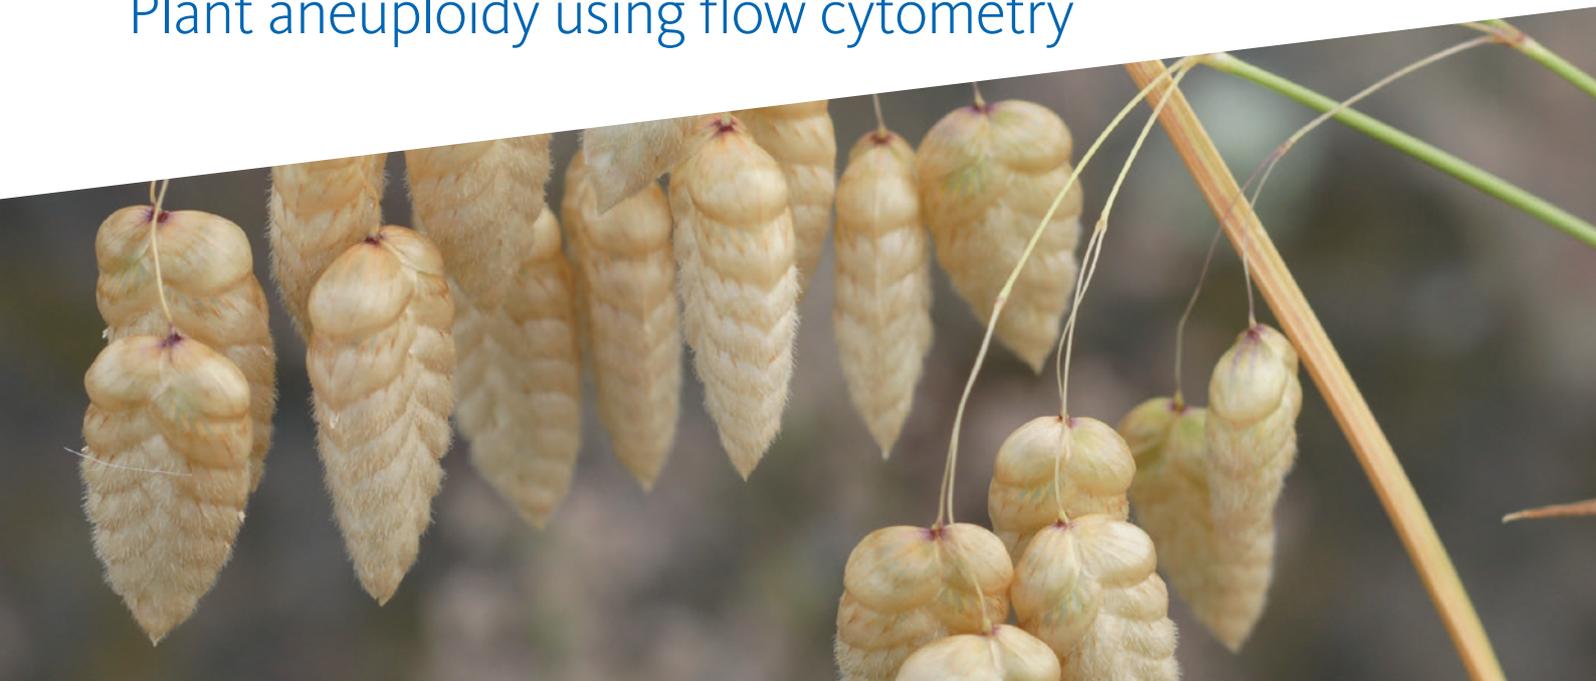

Background

Aneuploidy is defined as the addition or deletion of chromosomes compared to the 'normal' number of chromosomes as a multiple of the haploid chromosome number. Aneuploidy is probably the most common type of chromosomal aberration in the plant kingdom.

Traditionally, detecting aneuploidy in plants has been carried out by microscopic chromosome counting of preparations of metaphase chromosomes. In many cases metaphase chromosomes are difficult or almost impossible to obtain or count due to the high number and/or small size of the chromosomes. The procedure of counting chromosomes is time-consuming and involves handling unpleasant reagents, such as strong acids.

Flow cytometry, on the other hand, is fast since it does not count chromosomes but rather quantifies true amounts of DNA. And since the reagents are system-contained, there is less interaction with biohazardous materials.

Sysmex offers a number of flow cytometry-based **high-resolution DNA analysis** systems, such as CyFlow® PA, CyFlow® Space & CyFlow® Space Autoloading Station. These analysers detect variations in the number of chromosomes by measuring the amount of DNA of each individual nucleus. The method

compares a standard, known ploidy (of the same species) with the sample of interest (the suspected aneuploid). Additions or reductions to the chromosome number necessarily lead to more or less DNA per nucleus, and therefore provide an indication of the existence or absence of aneuploidy.

Please note that it is highly impractical to use a normal ploidy standard of species X for analysing an aneuploid sample from species Y (as in different species the chromosome number might be identical but the amount of DNA – or chromosome size – can differ substantially). It is not possible to count chromosomes directly using flow cytometry.





Basic procedure of a different species

Ploidy analysis standard determination

Individual samples are prepared together with an internal reference plant of a different species. The internal reference should have a similar DNA content as the sample plant so that, in the DNA histogram, the sample peak and internal reference peak are close. For instance, if the internal reference DNA peak is positioned on channel 100, the sample plants DNA peak should be located in a range of +/- 50 channels from that internal reference peak.

The mean position (x-axis value) of both reference and sample has to be defined. The standard ratio ($ratio_{std}$) between a sample peak position (e.g. of a diploid standard (ch_{std}) and a reference peak position (ch_{ref}) is a constant

value. To obtain information on the mean value and standard deviation of this standard ratio ($ratio_{std} = ch_{std} / ch_{ref}$), five to ten repetitive analyses of the standard and reference have to be performed.

Table 1: Example of standard calculation $ratio_{std}$ mean and $ratio_{std}$ standard deviation with X as reference and Y as sample

Sample No.	ch_{std}	ch_{ref}	$ratio_{std}$
01	76.4	100.2	0.762
02	74.8	101.0	0.740
03	75.3	101.3	0.743
04	74.6	100.1	0.745
05	76.0	099.9	0.761
Mean			0.750 +/- 0.010

After analysing the ploidy standard mixed with the reference for establishing both $ratio_{std}$ mean and $ratio_{std}$ standard deviation, individual samples can be investigated for aneuploidy.

In this previous example, the $ratio_{std}$ mean is 0.750 with a standard deviation of +/- 0.010.

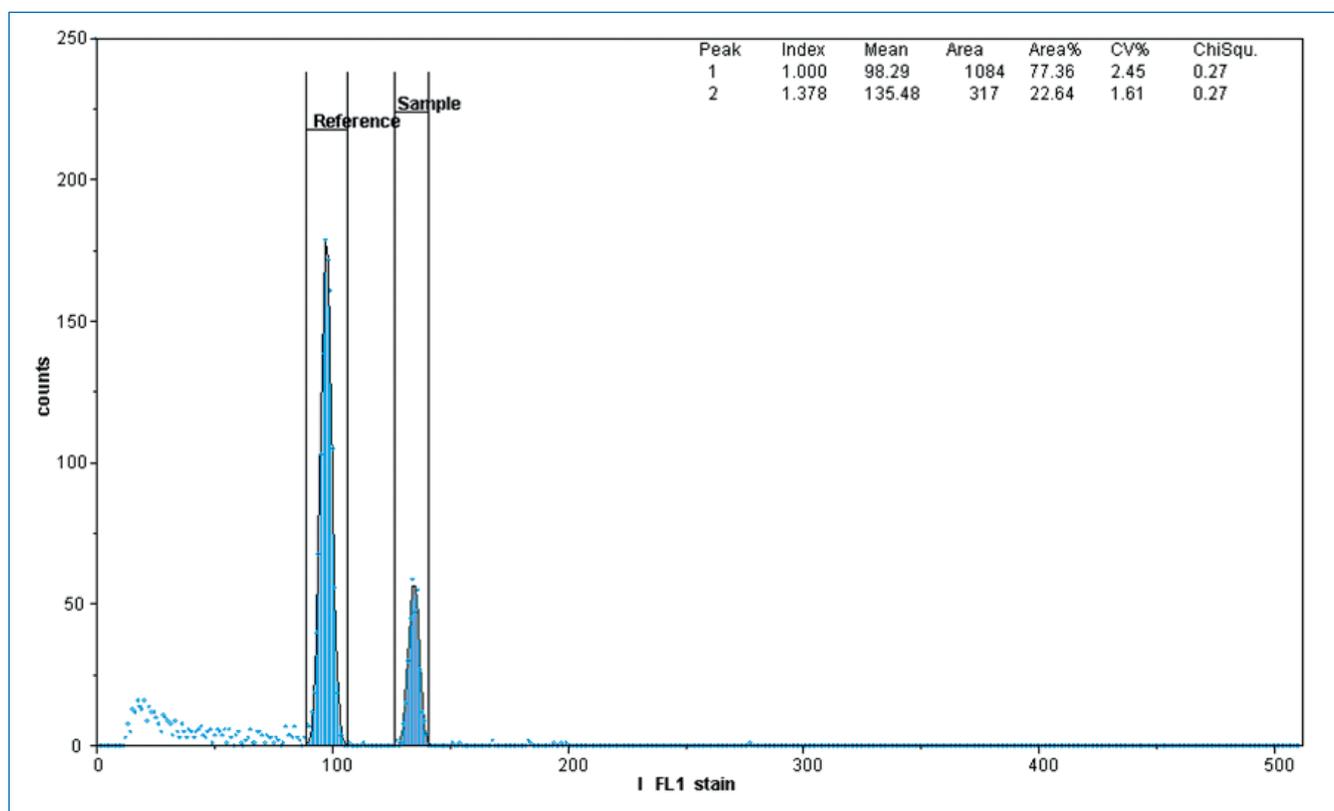


Figure 1: Nuclear DNA content analysis using a known plant as an internal reference. DNA peak is positioned on channel 100. Ideally, the sample plants DNA peak is located within +/- 50 channels from that internal reference peak.



Material solutions for aneuploidy analysis

Flow cytometry-based analysis for aneuploidy needs analyser configurations and reagents that are suited specifically to the complexity and characteristic of the sample DNA in question. Most samples can be analysed using the basic reagent (CyStain® UV Precise P). The remaining samples are analysed using more specialised, targeted solutions.

Table 3: Reagents

Reagent	Sysmex Order Codes	Fitting configuration
CyStain® UV Precise P	05-5002	for UV excitation (UV LED or laser), for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS07) ■ CyFlow® Ploidy Analyser (CY-S-3039_V1)
CyStain® UV Precise T	05-5003	for UV excitation (UV LED or laser), for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS07) ■ CyFlow® Ploidy Analyser (CY-S-3039_V1)
CyStain® UV Precise P automate	05-5002-a	for UV excitation (UV LED or laser), for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS07) with Autoloading Station
CyStain® UV Precise T automate	05-5003-a	for UV excitation (UV LED or laser), for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS07) with Autoloading Station
CyStain® PI Absolute P	05-5022	optimal for flow cytometer configurations with green (532 nm) or suitable with blue (488 nm) laser excitations for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS08) ■ CyFlow® Ploidy Analyser (CY-S-3039_V2)
CyStain® PI Absolute T	05-5023	optimal for flow cytometer configurations with green (532 nm) or suitable with blue (488 nm) laser excitations for example <ul style="list-style-type: none"> ■ CyFlow® Space (CY-S-3001R_VS08) ■ CyFlow® Ploidy Analyser (CY-S-3039_V2)

Sysmex also provides other consumables for the analysis process.

Table 4: Consumables

Material	Sysmex Order Codes
Petri dishes	04-2005
30 µm mesh CellTrics® filter	04-0042-2316
3.5 mL polystyrene sample tube	04-2000
DNA Control UV	05-7302
DNA Control PI	05-7303

Literature

- [1] **Doležal J, Goehde W.** (1995): Sex determination in dioecious plants *Melandrium album* and *M. rubrum* using high-resolution flow cytometry. *Cytometry*, , 19: 103–106.
- [2] **Doležal J, Greilhuber J, Suda J.** *Flow Cytometry with Plants: an overview. Flow Cytometry with Plant Cells.* Copyright® 2007 WILEY-VCH Verlag GmbH & Co. KGaA, Weinheim, ISBN: 978-3-527-31487.

Example aneuploidy analysis procedure

Each individual sample preparation mixed and stained with the reference plant has to follow the identical staining protocol as used to define the standard ratio. For each sample, calculate the sample ratio ($\text{ratio}_{\text{sample}} = \text{ch}_{\text{sample}} / \text{ch}_{\text{ref}}$) and $\Delta \text{ratio} = \text{ratio}_{\text{sample}} - \text{ratio}_{\text{std}}$.

Samples with a Δratio exceeding the standard deviation of the $\text{ratio}_{\text{std}}$ are suspected of aneuploidy. The higher the value of Δratio , the higher the probability of the sample being aneuploid.

Table 2: Example of sample calculation $\text{ratio}_{\text{sample}}$ and Δratio with X as reference and Y as sample. Δratio values shown in red exceed the $\text{ratio}_{\text{std}}$ standard deviation of ± 0.010 .

Sample No.	$\text{ch}_{\text{sample}}$	ch_{ref}	$\text{ratio}_{\text{sample}}$	$\text{ratio}_{\text{std}}$	Δratio	% DNA
s1	74.9	101.0	0.742	0.750	-0.008	98.9
s2	74.3	99.8	0.745	0.750	-0.005	99.3
s3	79.1	100.4	0.788	0.750	+0.038	105.1
s4	74.0	100.5	0.736	0.750	-0.014	98.1
s5	75.1	99.8	0.753	0.750	+0.003	100.4

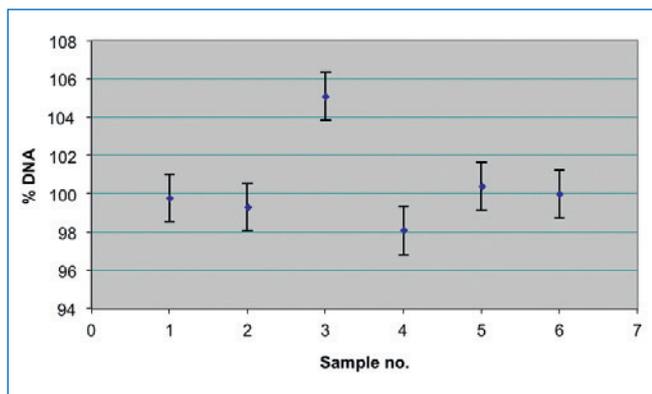


Figure 2: Chart displaying the percentage variation of DNA for every sample.

Case interpretation

Given a chromosome number of 24 chromosomes in a $2n$ plant (diploid), a statistical mean DNA difference of about 4.1% can be expected for the deletion or addition of a single chromosome (as one average chromosome represents 4.1% of total DNA). Therefore, 4.1% variation of the $\text{ratio}_{\text{std}}$ would correspond to 0.750 ± 0.031 . When Δratio strongly exceeds the $\text{ratio}_{\text{std}}$ standard deviation of 0.010, aneuploidy would be detected with high accuracy.

Naturally, the standard sample can be a different ploidy level ($3n$, $4n$, $6n$). If aneuploidy occurs in a different level of ploidy, it could also be detected.

For this case, in our previous example the $\text{ratio}_{\text{sample}}$ of sample s3 and s4 differs significantly from the analysis of the diploid standard and from the rest of the samples.

These results indicate that sample s3 ($\Delta \text{ratio} = +0.038$) encloses 25 chromosomes instead of 24 with similar mean standard deviation of a chromosome (± 0.031). Sample s3 can be considered aneuploid by the addition of a single chromosome ($s3 = 2n + 1$). Sample s4 shows ($\Delta \text{ratio} = -0.014$) a less significant deviation from the diploid standard. It might be considered aneuploid due to the deletion of one chromosome.

The result of such individual analysis should be verified by repeating the analysis of the suspect aneuploid plant.

Since the system does not count chromosomes, the final scientific verification can only be carried out by light microscopy and counting chromosomes. Aberrations in the DNA content can also occur by the addition of DNA during DNA exchange between single chromosomes without increasing their total number.

Please note that, if the total number of chromosomes is very high and/or the samples cannot be analysed with an acceptable level of reproducibility, detecting aneuploid plants with one chromosome more or less is uncertain. The $\text{ratio}_{\text{std}}$ standard deviation of repetitive analysis would be higher than the Δratio standard deviation, systematically leading to the interpretation of the addition/deletion of chromosomes.



Report examples

CyFlow® Space for aneuploidy analysis

Example: wheat sample aneuploidy analysis report with FloMax® software displaying fluorescence mean intensity of the sample and reference as well as a calculation of the Ratio and % DNA.

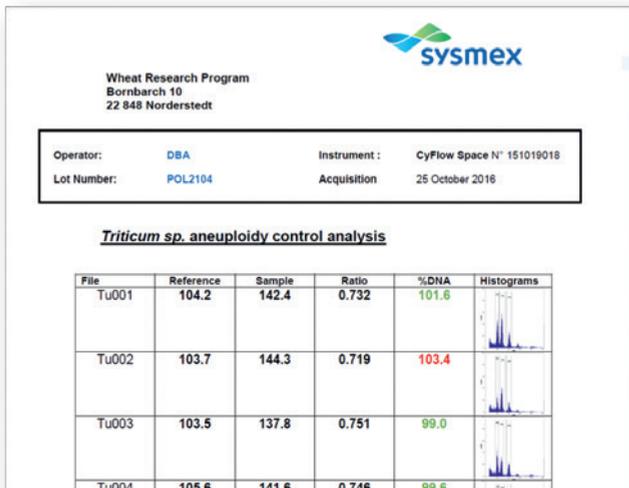


Figure 3: Wheat sample aneuploidy analysis – tube Tu002 is likely to be an aneuploid sample

CyFlow® Space Autoloading Station for aneuploidy

Example: aneuploidy analysis with CyPAD® software of a sample of cabbage. The report generated by Excel using data produced by a system with autoloading station conveniently offers the option of selecting different variables to adequately select undesirable specimens in regenerants from in vitro plant culture for instance.

In this example, three outliers in the graph are clearly aneuploid samples.

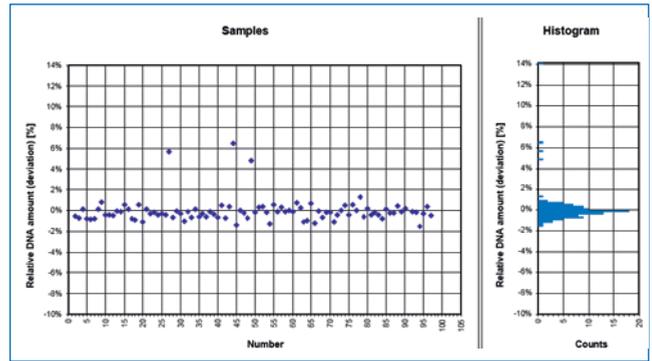


Figure 4: Cabbage sample aneuploidy analysis – histogram page clearly shows three outliers (aneuploid samples).

In the following image, open fields are used to fine-tune the aneuploidy experiments: position of the reference and expected variation as well as the calculated deviation of the reference.

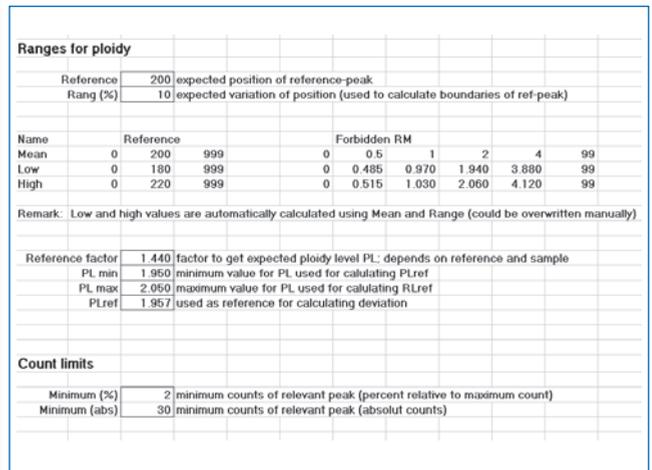


Figure 5: Cabbage sample aneuploidy analysis – user-definable page to input and fine-tune aneuploidy analysis report criteria

A general aneuploidy report including the 96-well cabbage samples is also generated.

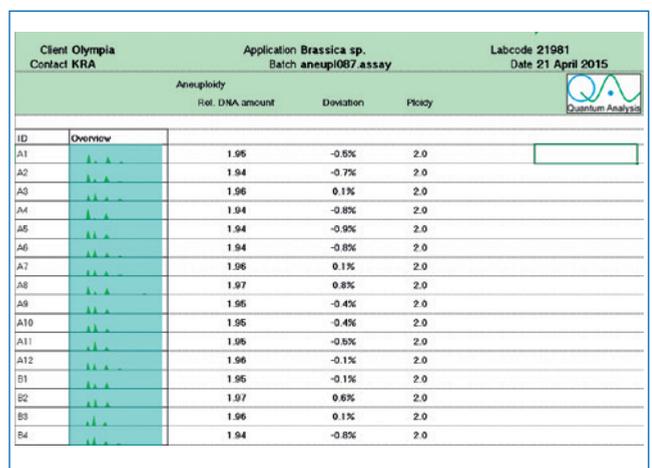


Figure 6: Cabbage sample aneuploidy analysis – result page displaying individual histograms, DNA amount and ploidy level

*Windows is a trademark or registered trademark of Microsoft Corporation in the United States and other countries.
Other company names and product names in the manual (here application note) are trademarks of their respective owners.
The fact that a trademark is not explicitly indicated in this manual (here application note) does not authorize its use. TM and ©
are not explicitly indicated in the manuals (here application note).*

Authorised representative: Sysmex Europe GmbH

Bornbarch 1, 22848 Norderstedt, Germany · Phone +49 40 52726-0 · Fax +49 40 52726-100 · info@sysmex-europe.com · www.sysmex-europe.com

Manufacturer: Sysmex Partec GmbH

Am Flugplatz 13, 02828 Görlitz, Germany · Phone +49 3581 8746-0 · Fax +49 3581 8746-70 · info@sysmex-partec.com · www.sysmex-partec.com

Sysmex Corporation

1-5-1 Wakinohama-Kaigandori, Chuo-ku, Kobe 651-0073, Japan · Phone +81 78 265-0500 · Fax +81 78 265-0524 · www.sysmex.co.jp